



Company Name: Vital Images  
Product Name: Vitrea View 7.4  
DICOM Conformance Statement  
Internal Document Number: VLC-10042 A  
Date: March 5, 2019

**IMPORTANT**

1. No part of this document may be copied or reprinted, in whole or in part, without written permission of Vital Images, Inc.
2. The contents of this document are subject to change without prior notice and without legal obligation.

## 1 Conformance Overview

This conformance statement applies to the following products:

- Vitrea View

The application supports the ability to query remote systems for a list of DICOM objects that may be retrieved.

Table 1-1 defines the SOP Classes to be loaded and viewed. Table 1-2 defines the set of DICOMweb services supported.

**Table 1-1 Viewable SOP Classes**

SOP Classes	SOP Class UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1
Digital Intra-Oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-Oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
CT Image Storage	1.2.840.10008.5.1.4.1.1.2
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
MR Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-frame Grayscale Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1
Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radio fluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128

RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

**Table 1-2 DICOMWeb Services**

Network Service	User of Service (User Agent)	Provider of Service (Origin Server)
<b>WADO-RS</b>		
Retrieve Study	Yes	No
Retrieve Study Metadata	Yes	No
Retrieve Frames	Yes	No
Retrieve Bulk Data	Yes	No
<b>QIDO-RS</b>		
Search For Studies	Yes	No
<b>STOW-RS</b>		
Store Instances	Yes	No

## Contents

<b>1</b>	<b>CONFORMANCE OVERVIEW .....</b>	<b>3</b>
<b>2</b>	<b>INTRODUCTION .....</b>	<b>7</b>
2.1	REVISION HISTORY .....	7
2.2	AUDIENCE .....	7
2.3	REMARKS .....	7
2.4	TERMS AND DEFINITIONS .....	8
2.5	BASICS OF DICOM COMMUNICATION.....	10
2.6	ABBREVIATIONS .....	11
2.7	REFERENCES.....	11
<b>3</b>	<b>IMPLEMENTATION MODEL .....</b>	<b>12</b>
3.1	VITREA VIEW APPLICATION DATA FLOW.....	12
3.2	FUNCTIONAL DEFINITION OF AE'S .....	13
3.2.1	<i>Functional Definition of Vitrea View AE.....</i>	<i>13</i>
<b>4</b>	<b>AE SPECIFICATIONS.....</b>	<b>14</b>
4.1	VITREA VIEW AE .....	14
4.1.1	<i>Vitre View AE SOP Classes .....</i>	<i>14</i>
4.1.2	<i>SOP Specific Conformance.....</i>	<i>14</i>
4.2	FIND-SCU.....	15
4.2.1	<i>SOP Classes.....</i>	<i>15</i>
4.2.2	<i>Association Policies.....</i>	<i>15</i>
4.2.3	<i>Association Initiation Policy.....</i>	<i>15</i>
4.2.4	<i>Association Acceptance Policy .....</i>	<i>18</i>
4.3	MOVE-SCU .....	19
4.3.1	<i>SOP Classes.....</i>	<i>19</i>
4.3.2	<i>Association Policies.....</i>	<i>19</i>
4.3.3	<i>Association Initiation Policy.....</i>	<i>19</i>
4.3.4	<i>Association Acceptance Policy .....</i>	<i>22</i>
4.4	QIDO-RS USER AGENT .....	23
4.4.1	<i>SOP Classes.....</i>	<i>23</i>
4.4.2	<i>Connection Policies.....</i>	<i>23</i>
4.4.3	<i>Association Initiation Policy.....</i>	<i>23</i>
4.4.4	<i>Association Acceptance Policy .....</i>	<i>24</i>
4.5	WADO-RS USER AGENT .....	25
4.5.1	<i>SOP Classes.....</i>	<i>25</i>
4.5.2	<i>Connection Policies .....</i>	<i>25</i>
4.5.3	<i>Association Initiation Policy.....</i>	<i>25</i>
4.5.4	<i>Association Acceptance Policy .....</i>	<i>25</i>
4.6	STOW-RS USER AGENT .....	26
4.6.1	<i>SOP Classes.....</i>	<i>26</i>
4.6.2	<i>Connection Policies .....</i>	<i>26</i>
4.6.3	<i>Association Initiation Policy.....</i>	<i>26</i>
4.6.4	<i>Association Acceptance Policy .....</i>	<i>26</i>
<b>5</b>	<b>NETWORK INTERFACES .....</b>	<b>27</b>
5.1	PHYSICAL NETWORK INTERFACE .....	27
5.2	ADDITIONAL PROTOCOLS .....	27
<b>6</b>	<b>CONFIGURATION .....</b>	<b>28</b>
6.1	AE TITLE/PRESENTATION ADDRESS MAPPING .....	28

---

6.2	PARAMETERS.....	28
7	SUPPORT OF CHARACTER SETS.....	29
8	SECURITY .....	30
8.1	NETWORK.....	30

## TABLE OF TABLES AND FIGURES

Table 1-1	Viewable SOP Classes .....	3
Table 1-2	DICOMWeb Services .....	4
Table 4-1	SOP Classes Supported by FIND-SCU.....	15
Table 4-2	DICOM Application Context for FIND-SCU.....	15
Table 4-3	Maximum PDU Size Sent for FIND-SCU .....	15
Table 4-4	Number of Associations for FIND-SCU.....	15
Table 4-5	DICOM Implementation Class and Version for FIND-SCU .....	15
Table 4-6	Proposed Presentation Contexts for FIND-SCU and Query Remote AE .....	16
Table 4-7	Study Root Request Identifier for FIND-SCU .....	17
Table 4-8	Response Status for FIND-SCU and Query Remote AE Request .....	17
Table 4-9	SOP Classes Supported by MOVE-SCU .....	19
Table 4-10	DICOM Application Context for MOVE-SCU .....	19
Table 4-11	Maximum PDU Size Sent for MOVE-SCU .....	19
Table 4-12	Number of Associations for MOVE-SCU .....	19
Table 4-13	DICOM Implementation Class and Version for MOVE-SCU .....	19
Table 4-14	Proposed Presentation Contexts for MOVE-SCU and Retrieve from Remote AE.....	20
Table 4-15	Study Root Request Identifier for MOVE-SCU.....	20
Table 4-16	Response Status for MOVE-SCU and Retrieve from Remote AE Request.....	21
Table 4-17	Transactions Supported by WADO-RS Origin Server .....	23
Table 4-18	QIDO-RS Specification .....	23
Table 4-19	Number of Associations for FIND-SCU.....	23
Table 4-20	QIDO-RS Query Parameters.....	23
Table 4-21	Transactions Supported by WADO-RS User Agent.....	25
Table 4-22	WADO-RS Specification.....	25
Table 4-23	Number of Associations for WADO-RS User Agent .....	25
Table 4-21	Transactions Supported by STOW-RS User Agent.....	26
Table 4-22	STOW-RS Specification.....	26
Table 4-23	Number of Associations for STOW-RS User Agent .....	26
Table 6-1	Configuration Parameters Table.....	28

## 2 Introduction

### 2.1 Revision History

REVISION	EFF Date	AUTHORS	CHANGES FROM PREVIOUS REVISION
A	28 February 2019	Tera Schultze	Initial Release

### 2.2 Audience

This document is written for the people that need to understand how Vitrea View will integrate into their healthcare facility. This includes both those responsible for overall imaging network policy and architecture, as well as integrators who need to have a detailed understanding of the DICOM features of the product. This document contains some basic DICOM definitions so that any reader may understand how this product implements DICOM features. However, integrators are expected to fully understand all the DICOM terminology, how the tables in this document relate to the product’s functionality, and how that functionality integrates with other devices that support compatible DICOM features. Also note that this document is formatted according to the DICOM 3.0 Specification, Part 2: Conformance.

### 2.3 Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between Vitrea View and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard. DICOM by itself does not guarantee interoperability. The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement is not supposed to replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, the user should be aware of the following important issues:

- The comparison of different Conformance Statements is just the first step towards assessing interconnectivity and interoperability between the product and other DICOM conformant equipment.
- Test procedures should be defined and executed to validate the required level of interoperability with specific compatible DICOM equipment, as established by the healthcare facility.

VitreView products participate in an industry-wide testing program sponsored by Integrating the Healthcare Enterprise (IHE). The IHE Integration Statement for Vitrea View, together with the IHE Technical Framework, may facilitate the process of validation testing.

## 2.4 Terms and Definitions

Informal definitions are provided for the following terms used in this Conformance Statement. The DICOM Standard is the authoritative source for formal definitions of these terms.

**Abstract Syntax** – the information agreed to be exchanged between applications, generally equivalent to a Service/Object Pair (SOP) Class. Examples: Verification SOP Class, Modality Worklist Information Model Find SOP Class, Computed Radiography Image Storage SOP Class.

**Application Entity (AE)** – an end point of a DICOM information exchange, including the DICOM network or media interface software; i.e., the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.

**Application Entity Title** – the externally known name of an Application Entity, used to identify a DICOM application to other DICOM applications on the network.

**Application Context** – the specification of the type of communication used between Application Entities. Example: DICOM network protocol.

**Association** – a network communication channel set up between Application Entities.

**Digital Imaging and Communications in Medicine (DICOM)** - DICOM is a global Information-Technology standard used in all hospitals worldwide.

**Information Object Definition (IOD)** – the specified set of *Attributes* that comprise a type of data object; does not represent a specific instance of the data object, but rather a class of similar data objects that have the same properties. The *Attributes* may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3), and there may be conditions associated with the use of an Attribute (Types 1C and 2C). Examples: MR Image IOD, CT Image IOD, Print Job IOD.

**Integrating the Healthcare Enterprise (IHE)** - IHE is an initiative by healthcare professionals and industry to improve the way computer systems in healthcare share information. IHE promotes the coordinated use of established standards such as DICOM and HL7 to address specific clinical need in support of optimal patient care.

**Joint Photographic Experts Group (JPEG)** – a set of standardized image compression techniques, available for use by DICOM applications.

**Media Application Profile** – the specification of DICOM information objects and encoding exchanged on removable media (e.g., CDs).

**Module** – a set of *Attributes* within an *Information Object Definition* that are logically related to each other. Example: Patient Module includes Patient Name, Patient ID, Patient Birth Date, and Patient Sex.

**Negotiation** – first phase of Association establishment that allows Application Entities to agree on the types of data to be exchanged and how that data will be encoded.

**Presentation Context** – the set of DICOM network services used over an Association, as negotiated between Application Entities; includes Abstract Syntaxes and Transfer Syntaxes.

**Protocol Data Unit (PDU)** – a packet (piece) of a DICOM message sent across the network. Devices must specify the maximum size packet they can receive for DICOM messages.

**Security Profile** – a set of mechanisms, such as encryption, user authentication, or digital signatures, used by an *Application Entity* to ensure confidentiality, integrity, and/or availability of exchanged DICOM data.



**Service Class Provider (SCP)** – role of an *Application Entity* that provides a DICOM network service; typically, a server that performs operations requested by another *Application Entity (Service Class User)*. Examples: Picture Archiving and Communication System (image storage SCP, and image query/retrieve SCP), Radiology Information System (modality worklist SCP).

**Service Class User (SCU)** – role of an *Application Entity* that uses a DICOM network service; typically, a client. Examples: imaging modality (image storage SCU, and modality worklist SCU), imaging workstation (image query/retrieve SCU).

**Service/Object Pair (SOP) Class** – the specification of the network or media transfer (service) of a particular type of data (object); the fundamental unit of DICOM interoperability specification. Examples: Ultrasound Image Storage Service, Basic Grayscale Print Management.

**Tag** – a 32-bit identifier for a data element, represented as a pair of four digit hexadecimal numbers, the “group” and the “element”. If the “group” number is odd, the tag is for a private (manufacturer-specific) data element. Examples: 0010,0020 [Patient ID], (07FE,0010) [Pixel Data], (0019,0210) [private data element].

**Transfer Syntax** – the encoding used for exchange of DICOM information objects and messages. Examples: *JPEG* compressed (images), little endian explicit value representation.

**Unique Identifier (UID)** – a globally unique “dotted decimal” string that identifies a specific object or a class of objects; an ISO-8824 Object Identifier. Examples: Study Instance UID, SOP Class UID, SOP Instance UID.

**Value Representation (VR)** – the format type of an individual DICOM data element, such as text, an integer, a person’s name, or a code. DICOM information objects can be transmitted with either explicit identification of the type of each data element (Explicit VR), or without explicit identification (Implicit VR); with Implicit VR, the receiving application must use a DICOM data dictionary to look up the format of each data element.

## 2.5 Basics of DICOM Communication

This section describes terminology used in this Conformance Statement for the non-specialist. The key terms used in the Conformance Statement are highlighted in *italics* below. This section is not a substitute for training about DICOM, and it makes many simplifications about the meanings of DICOM terms.

Two *Application Entities* (devices) that want to communicate with each other over a network using DICOM protocol must first agree on several things during an initial network “handshake”. One of the two devices must initiate an *Association* (a connection to the other device), and ask if specific services, information, and encoding can be supported by the other device (*Negotiation*).

DICOM specifies a number of network services and types of information objects, each of which is called an *Abstract Syntax* for the Negotiation. DICOM also specifies a variety of methods for encoding data, denoted *Transfer Syntaxes*. The Negotiation allows the initiating Application Entity to propose combinations of Abstract Syntax and Transfer Syntax to be used on the Association; these combinations are called *Presentation Contexts*. The receiving Application Entity accepts the Presentation Contexts it supports.

For each Presentation Context, the Association Negotiation also allows the devices to agree on *Roles* – which one is the *Service Class User* (SCU - client) and which is the *Service Class Provider* (SCP - server). Normally the device initiating the connection is the SCU, i.e., the client system calls the server, but not always.

The Association Negotiation finally enables exchange of maximum network packet (*PDU*) size, security information, and network service options (called *Extended Negotiation* information).

The Application Entities, having negotiated the Association parameters, may now commence exchanging data. Common data exchanges include queries for worklists and lists of stored images, transfer of image objects and analyses (structured reports), and sending images to film printers. Each exchangeable unit of data is formatted by the sender in accordance with the appropriate *Information Object Definition*, and sent using the negotiated Transfer Syntax. There is a Default Transfer Syntax that all systems must accept, but it may not be the most efficient for some use cases. Each transfer is explicitly acknowledged by the receiver with a *Response Status* indicating success, failure, or that query or retrieve operations are still in process.

Two Application Entities may also communicate with each other by exchanging media (such as a CD-R). Since there is no Association Negotiation possible, they both use a *Media Application Profile* that specifies “pre-negotiated” exchange media format, Abstract Syntax, and Transfer Syntax.

## 2.6 Abbreviations

AE	Application Entity
AET	Application Entity Title
CD-R	Compact Disk Recordable
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
FSC	File-Set Creator
FSU	File-Set Updater
FSR	File-Set Reader
GSPS	Grayscale Softcopy Presentation State
HIS	Hospital Information System
HL7	Health Level 7 Standard
IHE	Integrating the Healthcare Enterprise
IOD	Information Object Definition
JPEG	Joint Photographic Experts Group
MR	Magnetic Resonance Imaging
MSPS	Modality Scheduled Procedure Step
NM	Nuclear Medicine
PACS	Picture Archiving and Communication System
PET	Positron Emission Tomography
PDU	Protocol Data Unit
QIDO	Query by ID for DICOM Objects
RS	RESTful Services
SC	Secondary Capture
SCP	Service Class Provider
SCU	Service Class User
SOP	Service-Object Pair
SPS	Scheduled Procedure Step
SR	Structured Reporting
TCP/IP	Transmission Control Protocol/Internet Protocol
US	Ultrasound
VA	VitreViewAdvanced (including VitreViewWorkstation)
VC	VitreViewCore
VIMS	Vital Image Management System
VL	Visible Light
VR	Value Representation
WADO	Web Access to DICOM Objects
XA	X-ray Angiography


## 2.7 References

NEMA PS3	DICOM Standard, available free at <a href="http://medical.nema.org/">http://medical.nema.org/</a>
IHE	IHE, further information available at <a href="http://www.ihe.net/">http://www.ihe.net/</a>
VLC-10105	VitreView 7.10 DICOM Conformance
VLC-09634	VitreView Data Stream 2.1 DICOM Conformance
Karos 2018.04.014	<b>VitreView Connection 7.4 DICOM Conformance</b> All Vital conformance documents available at <a href="http://www.vitalimages.com/customer-success-support-program/compliance-documents">http://www.vitalimages.com/customer-success-support-program/compliance-documents</a>

## 3 Implementation Model

### 3.1 Vitrea View Application Data Flow

Figure 3-2 Implementation Model

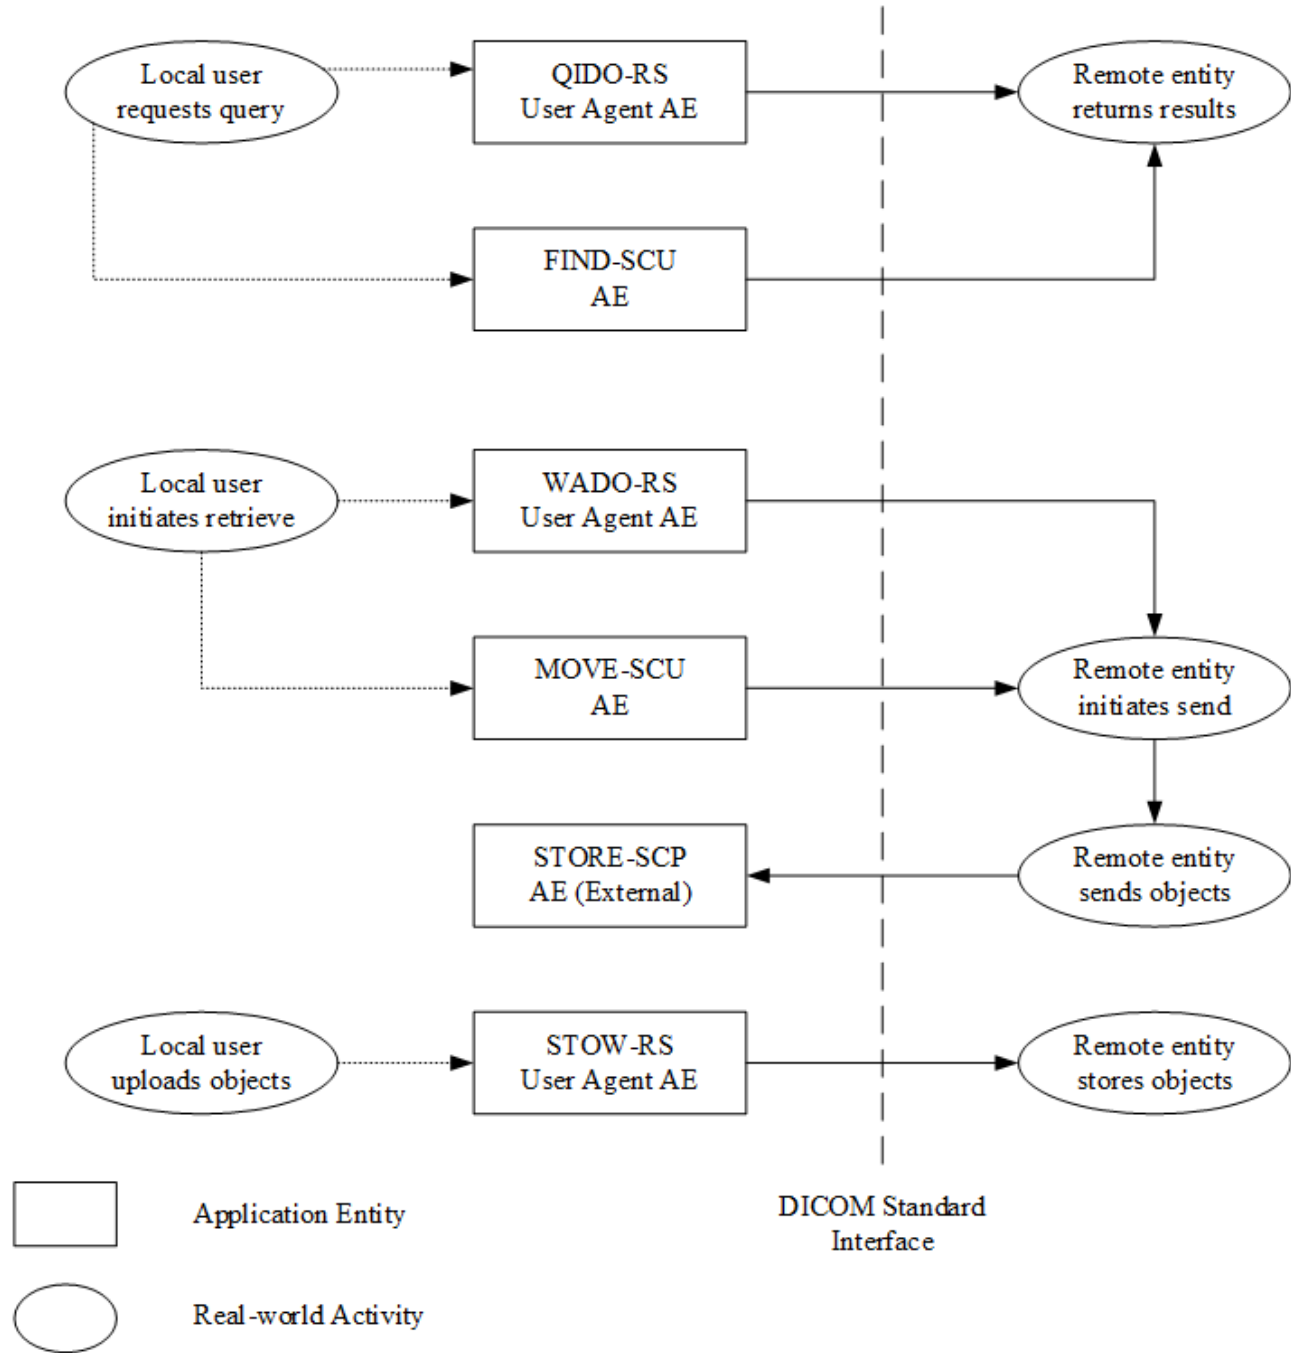

The implementation consists of a set of applications which provide a user interface, internal database and network listeners that spawn additional threads or processes as necessary to handle incoming connections.

Conceptually the network services may be modeled as the following separate AEs, though in fact some AEs share (configurable) AE Titles:

- FIND-SCU, which queries remote entities for lists of studies, series and instances
- QIDO-RS User Agent, which queries remote entities for lists of studies, series and instances
- STOW-RS UserAgent, which uploads DICOM studies to remote entities
- MOVE-SCU, which retrieves studies, series and instances from remote entities
- WADO-RS User Agent, which retrieves studies, series and instances from remote entities
- STORAGE-SCP (external), which receives images and other composite instances from remote entities

## 3.2 Functional Definition of AE's

### 3.2.1 Functional Definition of Vitrea View AE

The Vitrea View Application Entity interacts with one of the following Storage AEs:

- Vitrea Data Stream AE (see VLC-09634)
- Vitrea VNA Storage Server AE (see VLC-09563)
- VIMS AE (see VLC-09341)
- 3<sup>rd</sup> party AEs

The Vitrea View AE allows a user to view DICOM instances stored on one of the associated AEs.

The Vitrea View AE includes support for the following DICOM AEs:

#### 3.2.1.1 WADO-RS User Agent

WADO-RS is activated through the user interface when a user selects a study or series for retrieval. A connection to the WADO-RS Origin Server is established to retrieve the selected instances

#### 3.2.1.2 QIDO-RS User Agent

QIDO-RS is activated through the user interface when a user selects a QIDO-RS Origin Server to query (from a pre-configured list), then initiates a query. Queries are performed at the study level. A user can further expand each result in the query, which then initiates a series level query.

#### 3.2.1.3 STOW-RS User Agent

STOW-RS is activated through the user interface when a user imports data from media. Imported data is sent to a configured STOW-RS Origin Server.

#### 3.2.1.4 FIND-SCU

FIND-SCU is activated through the user interface when a user selects a remote AE to query (from a pre-configured list), then initiates a query. Queries are performed at the study level. A user can further expand each result in the query, which then initiates a series level query.

#### 3.2.1.5 MOVE-SCU

MOVE-SCU is activated through the user interface when a user selects a study or series for retrieval. A connection to the remote AE is established to initiate and monitor the retrieval while the associated Storage AE receives the retrieved instances.

## 4 AE Specifications

### 4.1 Vitrea View AE

#### 4.1.1 Vitrea View AE SOP Classes

The Vitrea View AE provides access to the following SOP Class(es): Table 1-1 Viewable SOP Classes.

#### 4.1.2 SOP Specific Conformance

This section describes any limitations to ViewView's ability to display standard SOP Classes.

The following modules are not supported:

- Overlay Plane

It is not possible to fully display instances containing these modules.

When displaying an image, a Grayscale Softcopy Presentation State or Color Softcopy Presentation State containing references to the image will be automatically applied in the following priority order:

1. A Presentation State referenced by the newest Key Object Selection instance referencing the image
2. The newest Grayscale Softcopy Presentation State or Color Softcopy Presentation State containing references to the image

The Vitrea View user has the option to select any other Presentation States that also references the image. If no Presentation State references the image then no Presentation State will be applied by default.

The following Grayscale Softcopy Presentation State / Color Softcopy Presentation State modules are not supported by Vitrea View:

- Presentation State Shutter
- Presentation State Mask
- Mask
- Display Shutter
- Bitmap Display Shutter
- Graphic Group
- Softcopy Presentation LUT

It is not possible to fully display Presentation States containing these modules.

The following Grayscale Softcopy Presentation State / Color Softcopy Presentation State attributes are supported by Vitrea View with some limitations:

- Presentation Size Mode (0070,0100): restricted to "SCALE TO FIT" and "MAGNIFY"
- Presentation Pixel Aspect Ratio (0070,0102): restricted to "1\1"
- Fill Mode (0070,0257): restricted to "SOLID"

It is not possible to fully display Presentation States containing other values for these attributes.

All of the Image Storage SOP Classes listed Table 1-1 are supported as references from instances of the Grayscale Softcopy Presentation State Storage SOP Class or of the Color Softcopy Presentation State.

## 4.2 FIND-SCU

### 4.2.1 SOP Classes

FIND-SCU provides Standard Conformance to the following SOP Class(es):

**Table 4-1 SOP Classes Supported by FIND-SCU**

SOP Class Name	SOP Class UID	SCU	SCP
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	No

### 4.2.2 Association Policies

#### 4.2.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 4-2 DICOM Application Context for FIND-SCU**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

**Table 4-3 Maximum PDU Size Sent for FIND-SCU**

Maximum PDU size sent	Unlimited, default is 65536
-----------------------	-----------------------------

#### 4.2.2.2 Number of Associations

**Table 4-4 Number of Associations for FIND-SCU**

Maximum number of simultaneous associations	1
---	---

#### 4.2.2.3 Asynchronous Nature

FIND-SCU will only allow a single outstanding operation on an Association. Therefore, FIND-SCU will not perform asynchronous operations window negotiation.

#### 4.2.2.4 Implementation Identifying Information

**Table 4-5 DICOM Implementation Class and Version for FIND-SCU**

Implementation Class UID	1.3.6.1.4.1.25403.1.1.1
Implementation Version Name	Dicom 0.1

### 4.2.3 Association Initiation Policy


FIND-SCU attempts to initiate a new association when the user initiates a query or searches a remote AE for priors.

#### 4.2.3.1 Activity – Query Remote AE

##### 4.2.3.1.1 Description and Sequencing of Activities

A single attempt will be made to query the remote AE. If the query fails, for whatever reason, no retry will be performed and the user is visually notified of the failure.

**Figure 4.1 Sequencing of Activity – Query Remote AE**

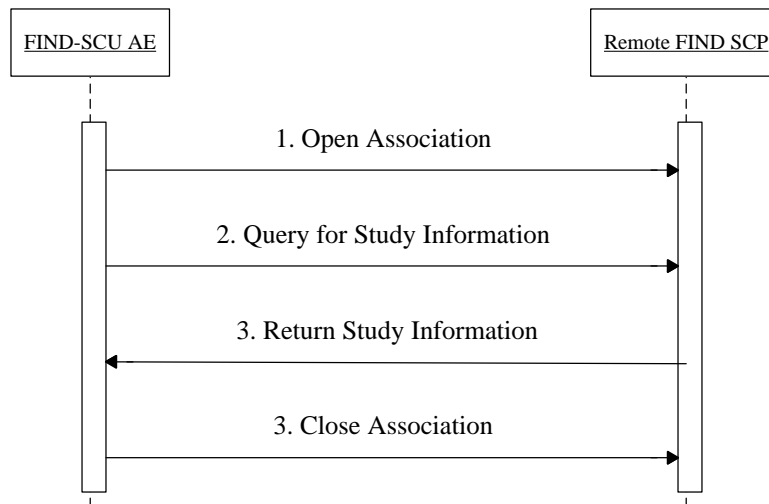

#### 4.2.3.1.2 Proposed Presentation Contexts

**Table 4-6 Proposed Presentation Contexts for FIND-SCU and Query Remote AE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Table 4-1 SOP Classes Supported by FIND-SCU	See Table 4-1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	Fuzzy Semantic Matching (optional)
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	Fuzzy Semantic Matching (optional)
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	Fuzzy Semantic Matching (optional)

FIND-SCU will propose a single Presentation Context, specified in the above table.

#### 4.2.3.1.3 Extended Negotiation

If configured, Fuzzy Semantic Matching will be requested. Relational queries are not supported.

#### 4.2.3.1.4 SOP Specific Conformance

##### 4.2.3.1.4.1 SOP Specific Conformance to C-FIND SOP Classes

FIND-SCU provides standard conformance to the supported C-FIND SOP Classes. Only a single information model, Study Root, is supported. Queries are initiated at the STUDY and SERIES levels, according to the request generated by the user interface. CANCEL requests are issued when the total number of matches exceeds the



configurable limit, to avoid overflow of data, where the default limit is 100 matches. Unexpected attributes returned in a C-FIND response (those not requested) are ignored. Requested return attributes not returned by the SCP will not cause a failure and will be interpreted as empty values, this will be logged for further information. Non-matching responses returned by the SCP due to unsupported (hopefully optional) matching keys are not filtered locally by the FIND-SCU and thus will still be presented in the worklist. Duplicate responses will replace existing entries in the display.

**Table 4-7 Study Root Request Identifier for FIND-SCU**

Name	Tag	Types of Matching
<b>STUDY Level</b>		
Study Date	(0008,0020)	*,U,R
Study Time	(0008,0030)	*,U,R
Accession Number	(0008,0050)	S,*,U
Modalities In Study	(0008,0061)	S,U
Referring Physician's Name	(0008,0090)	U
Study Description	(0008,1030)	U
Patient's Name	(0010,0010)	S,*,U
Patient's ID	(0010,0020)	S,*,U
Study Instance UID	(0020,000D)	UNIQUE
Study ID	(0020,0010)	U
Number of Study Related Instances	(0020,1208)	U
<b>SERIES Level</b>		
Series Date	(0008,0021)	U
Series Time	(0008,0031)	U
Modality	(0008,0060)	U
Series Description	(0008,103E)	U
Protocol	(0018,1030)	U
Series Instance UID	(0020,000E)	UNIQUE
Series Number	(0020,0011)	U
Number of Series Related Instances	(0020,1209)	U

Types of Matching:

- S Indicates the identifier attribute uses Single Value Matching
- R Indicates Range Matching
- \* Indicates wildcard matching
- U Indicates Universal Matching
- UNIQUE Indicates that this is the Unique Key for that query level, in which case Universal Matching or Single Value Matching is used depending on the query level.

**4.2.3.1.4.2 Presentation Context Acceptance Criterion**

FIND-SCU does not accept associations.

**4.2.3.1.4.3 Transfer Syntax Selection Policies**

FIND-SCU uses only Implicit Little Endian Transfer Syntax.

**4.2.3.1.4.4 Response Status**

FIND-SCU will behave as described in DICOM PS 3.2 Table D.4.2-24 in response to the status returned in the C-FIND response command message(s).

**Table 4-8 Response Status for FIND-SCU and Query Remote AE Request**

Service Status	Further Meaning	Status Codes	Behavior
Refused	Out of Resources	A700	Current query is terminated; remaining queries continue
Error	Identifier does not match SOP Class	A900	Current query is terminated; remaining queries continue
	Unable to process	Cxxx	Current query is terminated; remaining queries continue
Cancel	Matching terminated due to Cancel request	FE00	Current query is terminated; remaining queries continue
Success	Matching is complete - No final Identifier is supplied	0000	Query is successful
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier used to populate worklist
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this Identifier	FF01	Returned values not overridden

#### 4.2.4 Association Acceptance Policy

FIND-SCU does not accept associations.

## 4.3 MOVE-SCU

### 4.3.1 SOP Classes

MOVE-SCU provides Standard Conformance to the following SOP Class(es):

**Table 4-9 SOP Classes Supported by MOVE-SCU**

SOP Class Name	SOP Class UID	SCU	SCP
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No

### 4.3.2 Association Policies

#### 4.3.2.1 General

The DICOM standard application context name for DICOM 3.0 is always proposed:

**Table 4-10 DICOM Application Context for MOVE-SCU**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

**Table 4-11 Maximum PDU Size Sent for MOVE-SCU**

Maximum PDU size Sent	Unlimited, default of 65536
-----------------------	-----------------------------

#### 4.3.2.2 Number of Associations

**Table 4-12 Number of Associations for MOVE-SCU**

Maximum number of simultaneous associations	Configurable
---	--------------

#### 4.3.2.3 Asynchronous Nature

MOVE-SCU will only allow a single outstanding operation on an Association. Therefore, MOVE-SCU will not perform asynchronous operations window negotiation.

#### 4.3.2.4 Implementation Identifying Information

**Table 4-13 DICOM Implementation Class and Version for MOVE-SCU**

Implementation Class UID	1.3.6.1.4.1.25403.1.1.1
Implementation Version Name	Dicom 0.1

### 4.3.3 Association Initiation Policy


MOVE-SCU attempts to initiate a new association when the user initiates a retrieve from a remote device.

#### 4.3.3.1 Activity – Retrieve from Remote AE

##### 4.3.3.1.1 Description and Sequencing of Activities

For the entity (study or series) selected from the user interface to be retrieved, an attempt will be made to retrieve it from the selected remote AE. If the retrieve fails, for whatever reason, it will be retried every minute up to 3 times. This number of retries is configurable through the configuration tool.

**Figure 4.2 Sequencing of Activity – Retrieve from Remote AE**

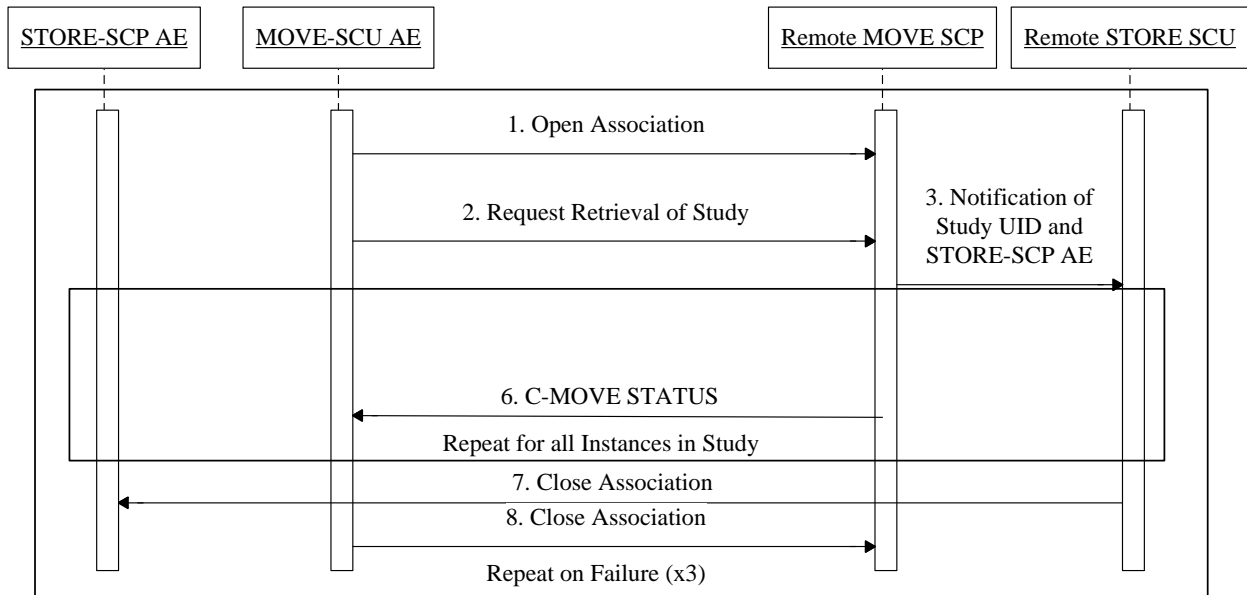

#### 4.3.3.1.2 Proposed Presentation Contexts

**Table 4-14 Proposed Presentation Contexts for MOVE-SCU and Retrieve from Remote AE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Table 4-9	See Table 4-9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

MOVE-SCU will propose a single Presentation Context.

#### 4.3.3.1.2.1 Extended Negotiation

No extended negotiation is performed. In particular, relational retrievals are not supported.

#### 4.3.3.1.3 SOP Specific Conformance

##### 4.3.3.1.3.1 SOP Specific Conformance to C-MOVE SOP Classes

MOVE-SCU provides standard conformance to the supported C-MOVE SOP Classes. Only a single information model, Study Root, is supported. Retrieval will be performed at the STUDY or SERIES level depending on what level of entity has been selected by the user in the browser. No CANCEL requests are ever issued.

The retrieval is performed from the AE that was specified in the Retrieve AE attribute returned from the query performed by FIND-SCU. The instances are retrieved to the current application’s local database by specifying the destination as the AE Title of the STORE-SCP AE of the local application. This implies that the remote C-MOVE SCP must be preconfigured to determine the presentation address corresponding to the STORE-SCP AE. The STORE-SCP AE will accept storage requests addressed to it from anywhere, so no pre-configuration of the local application to accept from the remote AE is necessary (except to configure the FIND-SCU).

**Table 4-15 Study Root Request Identifier for MOVE-SCU**

Name	Tag	Unique, Matching or Return Key
<b>STUDY level</b>		
Study Instance UID	(0020,000D)	U
<b>SERIES level</b>		
Series Instance UID	(0020,000E)	U

**4.3.3.1.3.2 Presentation Context Acceptance Criterion**

MOVE-SCU does not accept associations.

**4.3.3.1.3.3 Transfer Syntax Selection Policies**

MOVE-SCU uses only Implicit Little Endian Transfer Syntax.

**4.3.3.1.3.4 Response Status**

MOVE-SCU will behave as described in the Table below in response to the status returned in the C-MOVE response command message(s).

**Table 4-16 Response Status for MOVE-SCU and Retrieve from Remote AE Request**

Service Status	Further Meaning	Status Codes	Related Fields	Behavior
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)	Retrieval is terminated; Retries will occur
	Out of Resources - Unable to perform sub-operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)	Retrieval is terminated; Retries will occur
	Move Destination unknown	A801	(0000,0902)	Retrieval is terminated; Retries will occur
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)	Retrieval is terminated; Retries will occur
	Unable to process	Cxxx	(0000,0901) (0000,0902)	Retrieval is terminated; Retries will occur
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)	Retrieval is terminated; Retries will occur
Warning	Sub-operations Complete - One or more Failures	B000	(0000,1020) (0000,1022) (0000,1023)	Retrieval is terminated; Retry will occur
Success	Sub-operations Complete - No Failures	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)	Success of the retrieve
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)	Retrieval continues

**4.3.3.1.3.5 Sub-operation dependent behavior**

Since the C-MOVE operation is dependent on completion of C-STORE sub-operations that are occurring on a separate association, the question of failure of operations on the other association(s) must be considered.

MOVE-SCU completely ignores whatever activities are taking place in relation to the STORAGE-SCP AE that is receiving the retrieved instances. Once the C-MOVE has been initiated it runs to completion (or failure) as described in the C-MOVE response command message(s). There is no attempt by MOVE-SCU to confirm that instances have actually been successfully received or locally stored.

Whether or not completely or partially successfully retrievals are made available in the local database to the user is purely dependent on the success or failure of the C-STORE sub-operations, not on any explicit action by MOVE-SCU. If there are any failures that are recoverable, the retrieve will be retried up to a configurable limit, where the default is 3 times on a one minute interval.

If the association on which the C-MOVE was issued is aborted for any reason, whether or not the C-STORE sub-operations continue is dependent on the remote AE; the local STORAGE-SCP will continue to accept associations and storage operations regardless.

**4.3.4 Association Acceptance Policy**

MOVE-SCU does not accept associations.

## 4.4 QIDO-RS User Agent

### 4.4.1 SOP Classes

QIDO-RS User Agent supports the following transactions:

**Table 4-17 Transactions Supported by WADO-RS Origin Server**

Transaction	Resource
Search For Studies	{service}/studies?

### 4.4.2 Connection Policies

#### 4.4.2.1 General

QIDO-RS User Agent initiates associations based on user actions.

**Table 4-18 QIDO-RS Specification**

Category	Restrictions
Media Types supported	multipart/related; type=application/dicom+xml

#### 4.4.2.2 Number of Associations

**Table 4-19 Number of Associations for FIND-SCU**

Maximum number of simultaneous associations	1
---	---

#### 4.4.2.3 Asynchronous Nature

QIDO-RS User Agent will only allow a single outstanding operation on an Association. Therefore, FIND-SCU will not perform asynchronous operations window negotiation.

### 4.4.3 Association Initiation Policy

QIDO-RS User Agent attempts to initiate a new association when the user initiates a search from a QIDO-RS Origin Server.

#### 4.4.3.1 QIDO-RS Query Parameters

QIDO-RS User Agent supports the following search query keys.

**Table 4-20 QIDO-RS Query Parameters**

Name	Tag	Types of Matching
<b>STUDY Level</b>		
Study Date	(0008,0020)	*,U,R
Study Time	(0008,0030)	*,U,R
Accession Number	(0008,0050)	S,*,U
Modalities In Study	(0008,0061)	S,U
Study Description	(0008,1030)	U
Patient's Name	(0010,0010)	S,*,U
Patient's ID	(0010,0020)	S,*,U
Patient's Birth Date	(0010,0030)	U
Issuer of Patient ID	(0010,0021)	S,*,U

Study Instance UID	(0020,000D)	UNIQUE
Study ID	(0020,0010)	U
Number of Study Related Instances	(0020,1208)	U
<b>SERIES Level</b>		
Institution Name	(0008,0080)	S,*,U
<b>Other</b>		
Limit	N/A	N/A

Types of Matching:

- S Indicates the identifier attribute uses Single Value Matching
- R Indicates Range Matching
- \* Indicates wildcard matching
- U Indicates Universal Matching
- UNIQUE Indicates that this is the Unique Key for that query level, in which case Universal Matching or Single Value Matching is used depending on the query level.

**4.4.4 Association Acceptance Policy**

QIDO-RS User Agent does not accept associations.



## 4.5 WADO-RS User Agent

### 4.5.1 SOP Classes

WADO-RS User Agent supports the following transactions:

**Table 4-21 Transactions Supported by WADO-RS User Agent**

Transaction	Resource
Retrieve Study	{service}/studies/{StudyInstanceUID}
Retrieve Study Metadata	{service}/studies/{StudyInstanceUID}/metadata
Retrieve Frames	{service}/studies/{StudyInstanceUID}/series/{SeriesInstanceUID}/instances/{SOPInstanceUID}/frames/{frameList}
Retrieve Bulk Data	{bulkDataURL}

### 4.5.2 Connection Policies

#### 4.5.2.1 General

WADO-RS User Agent initiates associations based on user actions.

**Table 4-22 WADO-RS Specification**

Category	Restrictions
Media Types supported	multipart/related; type=application/dicom multipart/related; type=application/dicom+xml multipart/related; type=application/octet-stream
Transfer Syntaxes Supported	1.2.840.10008.1.2 (Implicit VR Little Endian) 1.2.840.10008.1.2.1 (Explicit VR Little Endian)
SOP Class Restrictions	Restricted to Storage SOP Classes specified in Table 1-1 Viewable SOP Classes.

#### 4.5.2.2 Number of Associations

**Table 4-23 Number of Associations for WADO-RS User Agent**

Maximum number of simultaneous associations	Unlimited
---	-----------

#### 4.5.2.3 Asynchronous Nature

WADO-RS User Agent will only make a single outstanding operation on an Association.

### 4.5.3 Association Initiation Policy

WADO-RS User Agent attempts to initiate a new association when the user initiates a retrieval from a WADO-RS Origin Server.

### 4.5.4 Association Acceptance Policy

WADO-RS User Agent does not accept associations.

## 4.6 STOW-RS User Agent

### 4.6.1 SOP Classes

STOW-RS User Agent supports the following transactions:

**Table 4-24 Transactions Supported by STOW-RS User Agent**

Transaction	Resource
Store Instances	{service}/studies

### 4.6.2 Connection Policies

#### 4.6.2.1 General

STOW-RS User Agent initiates associations based on user actions.

**Table 4-25 STOW-RS Specification**

Category	Restrictions
Media Types supported	multipart/related; type=application/dicom
Transfer Syntaxes Supported	1.2.840.10008.1.2 (Implicit VR Little Endian) 1.2.840.10008.1.2.1 (Explicit VR Little Endian)
SOP Class Restrictions	Restricted to Storage SOP Classes specified in Table 1-1 Viewable SOP Classes.

#### 4.6.2.2 Number of Associations

**Table 4-26 Number of Associations for STOW-RS User Agent**

Maximum number of simultaneous associations	Unlimited
---	-----------

#### 4.6.2.3 Asynchronous Nature

STOW-RS User Agent will only make a single outstanding operation on an Association.

### 4.6.3 Association Initiation Policy

STOW-RS User Agent attempts to initiate a new association when the user initiates an upload to a STOW-RS Origin Server.

### 4.6.4 Association Acceptance Policy

STOW-RS User Agent does not accept associations.

## 5 Network Interfaces

### 5.1 Physical Network Interface

The application is indifferent to the physical medium over which TCP/IP executes; which is dependent on the underlying operating system and hardware.

### 5.2 Additional Protocols

When host names rather than IP addresses are used in the configuration properties to specify presentation addresses for remote AEs, the application is dependent on the name resolution mechanism of the underlying operating system.

## 6 Configuration

Configuration is performed through the use of an administration tool. Refer to the product documentation for specific details.

### 6.1 AE Title/Presentation Address Mapping

All SCU requests are performed using the “local” AE. Each AE has an alias assigned to allow a user to easily distinguish AEs from each other. Aliases are configurable, and are generally human-readable strings. Presentation addresses (IP address and Port) are also configurable for all AEs.

### 6.2 Parameters

**Table 6-1 Configuration Parameters Table**

Parameter	Configurable	Default Value
<b>AE Specific Parameters (all AEs)</b>		
Number of retries on failure (MOVE-SCU AE, STORE-SCU AE, PRINT-SCU AE only)	Yes	3 (MOVE-SCU AE), 5 (STORE-SCU AE and PRINT-SCU AE)
Supported DIMSE services	Yes	None

## 7 Support of Character Sets

All Vital Images DICOM applications support ISO\_IR 100 (ISO 8859-1:1987 Latin Alphabet No. 1 supplementary set). No other character sets are supported.

## 8 Security

### 8.1 Network

Vitrea View can use HTTPS for WADO-RS, STOW-RS and QIDO-RS connections.

For DIMSE connections, Vitrea View does not support any specific network security measures. It is assumed the software is used within a secured environment. It is assumed that a secured environment includes at a minimum:

- Firewall or router protections to ensure that only approved external hosts have network access to the software.
- Firewall or router protections to ensure that the software only has network access to approved external hosts and services.
- Any communication with external hosts and services outside the locally secured environment use appropriate secure network channels (e.g. such as a Virtual Private Network (VPN)).

Other network security procedures such as automated intrusion detection may be appropriate in some environments. Additional security features may be established by the local security policy and are beyond the scope of this conformance statement.